

Fig. 1

**THE** **NEW** **YORK** **PUBLIC** **LIBRARY**

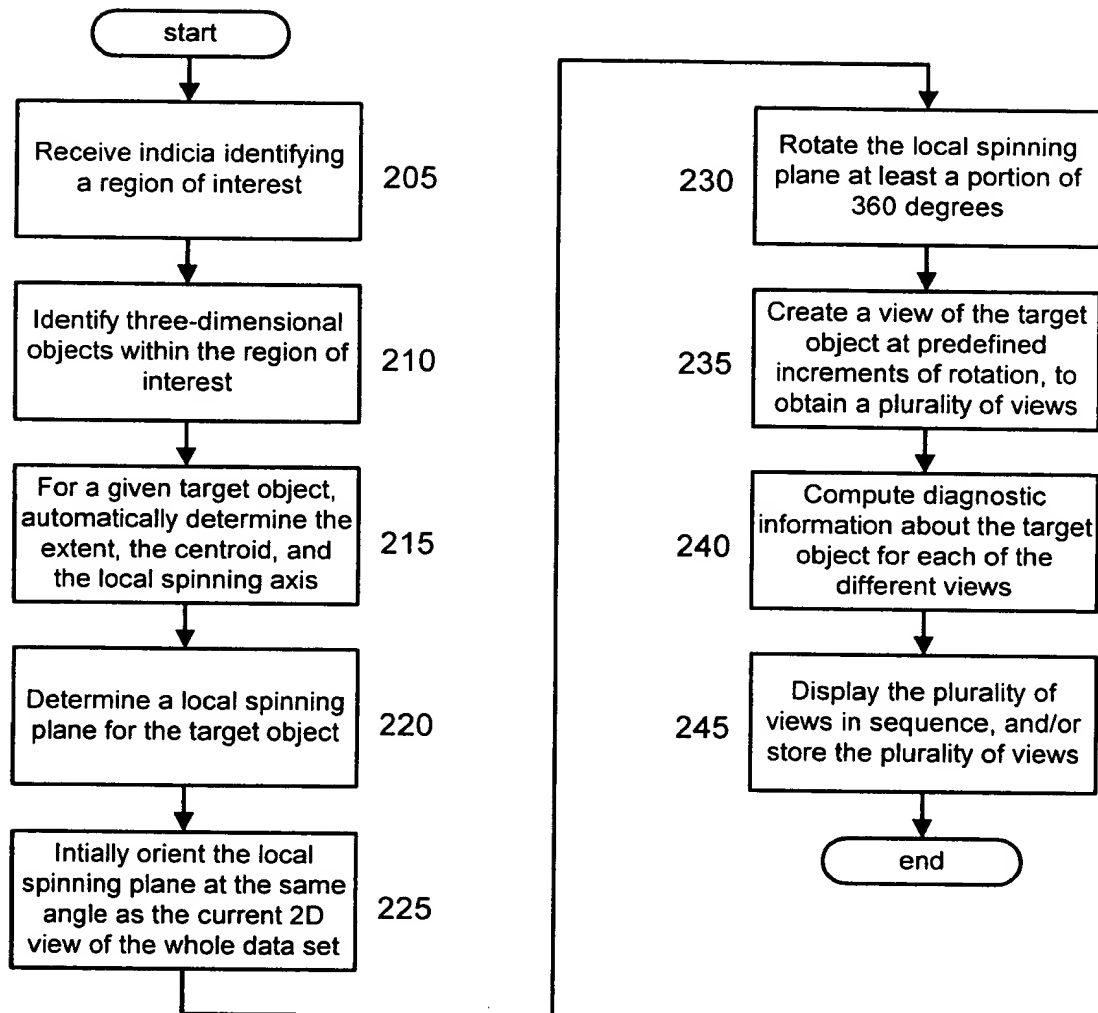


FIG. 2

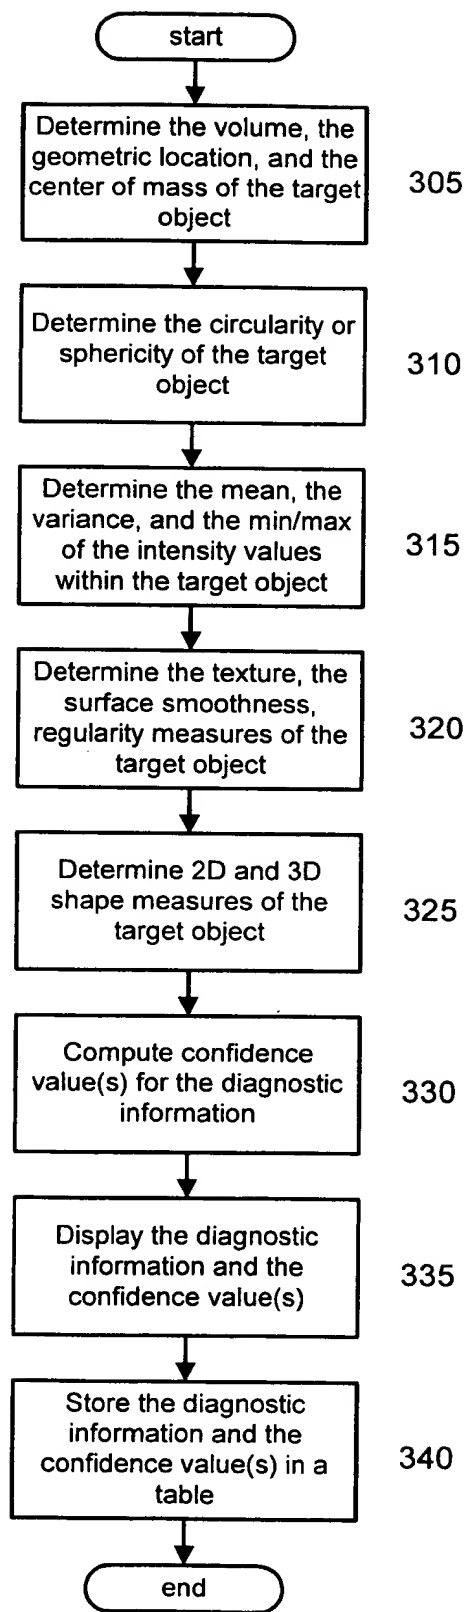


FIG. 3

```

graph TD
    Start([start]) --> 405[Set default thresholds for identifying features of the objects that may be suspicious]
    405 --> 410[Adjust default thresholds, as necessary]
    410 --> 415[Automatically identify objects that are suspicious, based on the thresholds]
    415 --> 420[Register the current data set with one or more data sets taken of the same patient at another time(s)]
    420 --> 425[Compare the data]
    425 --> 430[Output comparison result]
    430 --> End([end])

```

[illegible]

000290-4950950

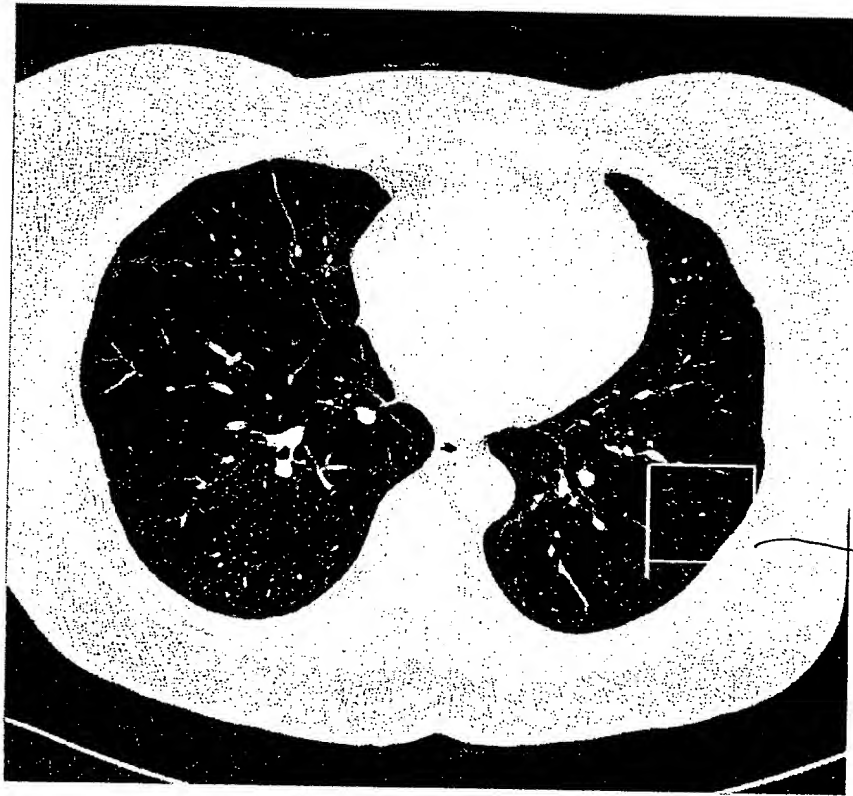


FIG. 5

510



FIG. 6

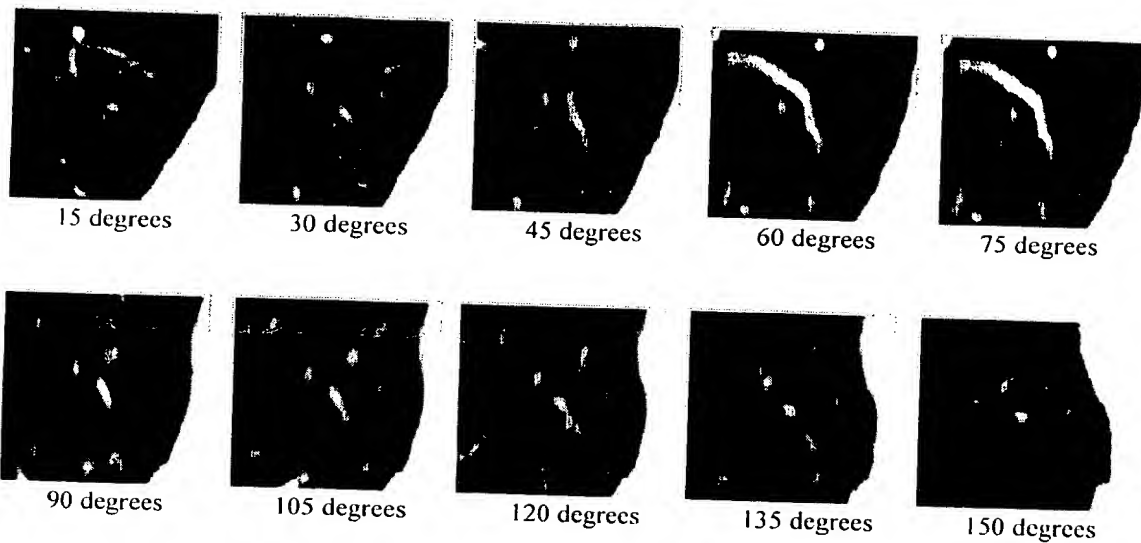


FIG. 7

00606564-062300